



Chlorine (Cl₂) or chlorine dioxide (ClO₂) sensor cube

- Fully compatible with büS systems and a wide range of further analysis sensor cubes
- Optional pH compensated chlorine measurement
- Hot swap compatible for exchanging the sensor cube during operation
- Minimal sample water consumption
- MEMS technology sensor

Product variants described in the data sheet may differ from the product presentation and description.

Can be combined with

	Type 8905	Online water analysis system
	Type 8906	Online water analysis system
	Type MS01	pH Sensor Cube
	Type MZ15	Manual calibration and cleaning module
	Type ME61	EDIP process display
	Type ME43	Fieldbus gateway
	Type ME63	Industrial Ethernet gateway, IP65/ IP67/ IP69k
	Type ME44	I/O module, IP 20
	Type ME66	büS distribution box, IP65/ IP67/ IP69k

Type description

This sensor cube measures the free acting chlorine or chlorine dioxide in the water, depending on the variant. The sensor cube is designed for operation on the fluidic backplane in the device Type 8905 online water analysis system.

The sensor cube contains a high precision membrane covered amperometric sensor, based on Bürkert MEMS technology (micro electro-mechanical system). The measurement shows the Cl₂ or ClO₂ content in the sample water. The chlorine sensor cube measures either the available chlorine HOCl or, if an MS01 pH sensor cube is connected for pH compensation, the free chlorine.

The electrical and fluidic connections are made via the backplane of the system. The sensor cube communicates with the system via the digital büS interface, allowing fully automatic login to the online water analysis system. If the sensor is plugged into the system, it automatically logs on to the büS and can be parameterised according to customer requirements.

As a supplement to the standard sensor, there is a variant with an external KCl reference electrode. This sensor is recommended for changing chlorine concentrations and generally unsteady process conditions.

Table of contents

1. General technical data	4
2. Approvals and conformities	5
2.1. Conformity	5
2.2. Standards.....	5
3. Materials	5
3.1. Bürkert resistApp.....	5
4. Dimensions	6
5. Product installation	7
5.1. Installation notes.....	7
6. Product design and assembly	7
6.1. Product features	7
7. Ordering information	8
7.1. Bürkert eShop	8
7.2. Bürkert product filter	8
7.3. Ordering chart	8
7.4. Ordering chart accessories.....	8

1. General technical data

Product properties

Material

Make sure the device materials are compatible with the fluid you are using.

Further information can be found in chapter ["3.1. Burkert resistApp" on page 4](#).

Further information can be found in chapter [PPE+PS](#)

Lever Zamak, painted
Seal EPDM

Compatibility With online water analysis system Type 8905 (the electrical and fluidic contact is made via backplane system.)
Further information can be found in the data sheet of the online water analysis system, see [data sheet Type 8905 ▶](#)

Dimensions Further information can be found in chapter ["4. Dimensions" on page 5](#).

Chlorine/chlorine dioxide sensor Membrane covered PT-cell, amperometric 3 electrodes measurement, without electrolyte

Temperature sensor Pt1000 Class B, no contact with the water sample

Measuring range

Chlorine measurement (Cl_2) 0.01...5 ppm
Chlorine dioxide measurement (ClO_2) 0.005...5 ppm

Maintenance 12 months nominal, depending on the water quality

Performance data

Chlorine measurement (Cl_2)

pH compensation Yes, with MS01 sensor cube
Further information can be found in the data sheet of the pH sensor cube, see [data sheet Type MS01 ▶](#)
Measurement deviation ± 0.03 ppm or ± 5 % of the measured value
Measuring range resolution 0.01 ppm
Linearity ± 0.02 ppm of the measured value
Repeatability ± 0.02 ppm of the measured value
Response time (t_{90}) < 30 s

Chlorine dioxide measurement (ClO_2)

pH compensation No
Measurement deviation ± 0.005 ppm or ± 3 % of the measured value (the greater value applies)
Measuring range resolution 0.001 ppm
Linearity ± 0.01 ppm or ± 3 % of the measured value (the greater value applies)
Repeatability ± 0.01 ppm or ± 3 % of the measured value (the greater value applies)
Response time (t_{90}) < 30 s

Temperature measurement

Measuring range 0...+ 50 °C (+ 32...+ 122 °F)
Measuring range resolution 0.01 °C (0.018 °F)

Electrical data

Operating voltage 24 V DC through the backplane of the system Type 8905 via büS
Power consumption 0.8 VA

Medium data

Fluid Water without particles: drinking water, industrial water
Fluid pH range pH 4...pH 9
Fluid conductivity > 50 $\mu\text{s}/\text{cm}$
Temperature of the fluid sample + 3...+ 40 °C (+ 37...+ 104 °F)
Pressure of the fluid sample PN 3
Flow rate of the fluid sample > 6 l/h

Product connections

Process connection Via pinch valve in the fluidic backplane of the Type 8905
Further information can be found in the data sheet of the online water analysis system, see [data sheet Type 8905 ▶](#)
Electrical connection Spring contacts in the fluidic backplane of the Type 8905, which is connected to a büS System
Further information can be found in the data sheet of the online water analysis system, see [data sheet Type 8905 ▶](#)

Data transfer

Internal communication	Through büS (Bürkert system bus, CANopen protocol)
External communication by status LED	According to NAMUR NE 107

Approvals and conformities**Directives**

CE directive	Further information on the CE directive can be found in chapter " 2.2. Standards " on page 4.
--------------	---------------------------------------------------------------------------------------------------------------

Environment and installation

Ambient temperature	<ul style="list-style-type: none"> Operation: +3...+40 °C (+37...+104 °F) Storage and transport: -10...+60 °C (+14...+140 °F), for empty/purged sensor cube
Relative air humidity	≤ 90%, without condensation
Height above sea level	Max. 2000 m
Operating condition	Continuous
Equipment mobility	Fixed
Application range	Indoor and outdoor Protect the device against electromagnetic interference, ultraviolet rays and, when installed outdoors, against the effects of climatic conditions.
Degree of protection according to IEC/EN 60529	<ul style="list-style-type: none"> IP65, when plugged in the fluidic backplane IP20, as standalone product
Installation category	Category I according to UL/EN 61010-1
Pollution degree	Degree 2 according to UL/EN 61010-1

2. Approvals and conformities

2.1. Conformity


In accordance with the Declaration of Conformity, the product is compliant with the EU Directives.

2.2. Standards

The applied standards which are used to demonstrate compliance with the EU Directives are listed in the EU-Type Examination Certificate and/or the EU Declaration of Conformity.

3. Materials

3.1. Bürkert resistApp

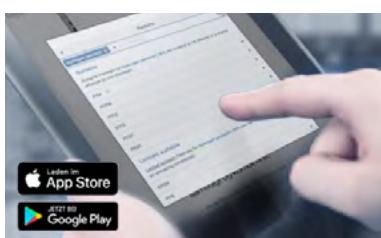

Bürkert resistApp – Chemical resistance chart

You want to ensure the reliability and durability of the materials in your individual application case? Verify your combination of media and materials on our website or in our resistApp.



[Start chemical resistance check](#)

4. Dimensions


Note:

Dimensions in mm, unless otherwise stated

Without external KCl reference electrode

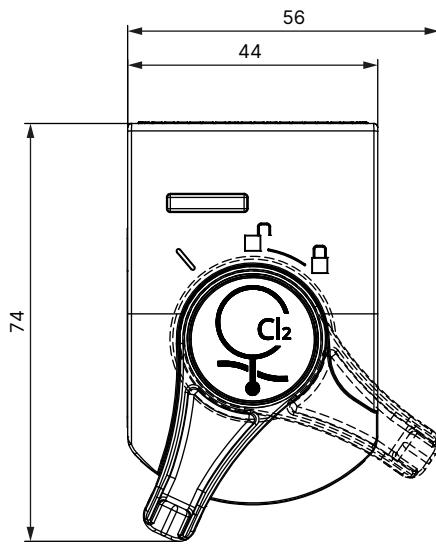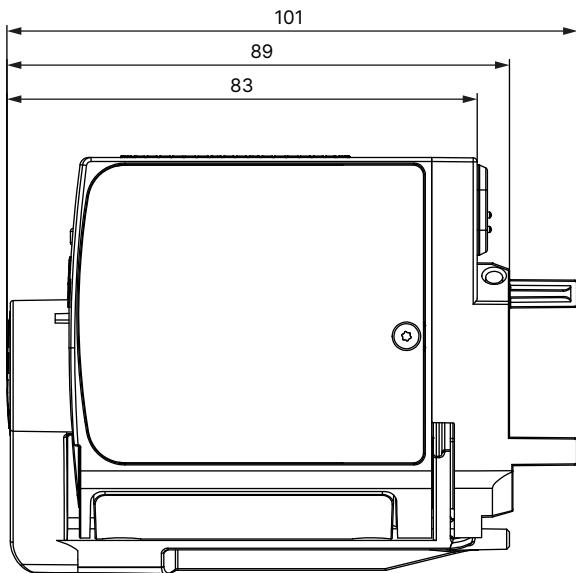

With external KCl reference electrode

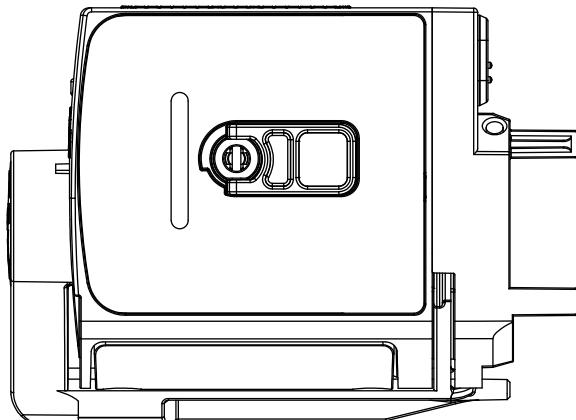


5. Product installation

5.1. Installation notes

The Type MS02 sensor cube is designed for use with the Type 8905 online water analysis system. The sensor cube is mounted onto the backplane of the Type 8905, which is installed on a standard DIN rail (TS35).


See **data sheet Type 8905** ▶ online water analysis system for more information.

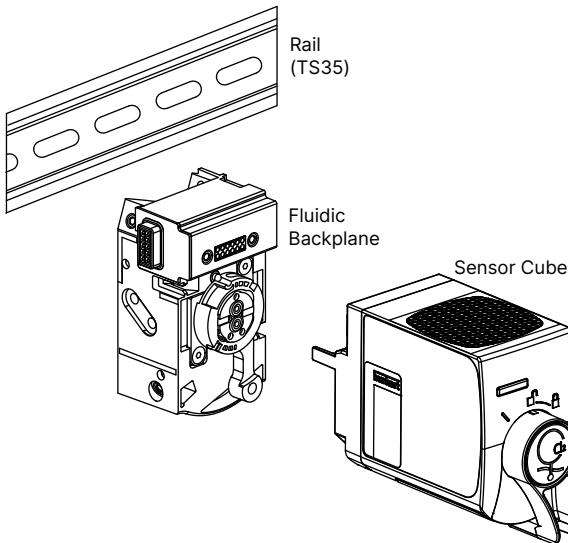


6. Product design and assembly

6.1. Product features

Without external KCl reference electrode

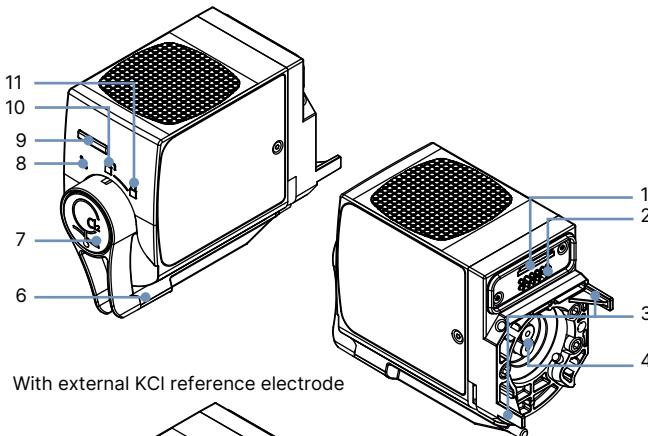

With external KCl reference electrode

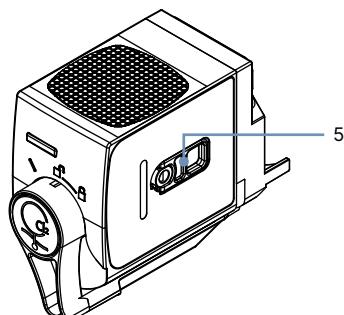

No.	Element
1	Slot micro-SIM card (for configuration data)
2	Electrical interface
3	Guide pins
4	Fluid connections
5	KCl reference electrode
6	Lever to: <ul style="list-style-type: none"> lock / unlock the product carry out maintenance operations
7	Push button for unlocking
8	Maintenance position
9	Sensor cube Status LED
10	Unlocked position
11	Locked position

7. Ordering information

7.1. Bürkert eShop



Bürkert eShop – Easy ordering and quick delivery

You want to find your desired Bürkert product or spare part quickly and order directly? Our online shop is available for you 24/7. Sign up and enjoy all the benefits.

[Order online now](#)

7.2. Bürkert product filter



Bürkert product filter – Get quickly to the right product

You want to select products comfortably based on your technical requirements? Use the Bürkert product filter and find suitable articles for your application quickly and easily.

[Try out our product filter](#)

7.3. Ordering chart

Note:

The chlorine/chlorine dioxide sensor cube must be operated within a system.

Observe the order information for online water analysis system Type 8905, see [data sheet Type 8905](#) ▶ or contact your Bürkert sales office.

Description	Article no.
Chlorine (Cl ₂) sensor cube	567625 ☰
Chlorine (Cl ₂) sensor cube with reference electrode	573205 ☰
Chlorine dioxide (ClO ₂) sensor cube	567721 ☰

7.4. Ordering chart accessories

Description	Article no.
Photometer MD100, measuring range 0.01...6 ppm	566393 ☰
DPD-1 reagent (100 tablets)	566394 ☰
Spare parts set: chlorine measuring cell	568040 ☰
KCl reference electrode	574042 ☰